

**LINSEIS**


T H E R M A L   A N A L Y S I S

**SIMULTANEOUS  
THERMAL  
ANALYSIS**

STA PT 1000

STA PT 1600

STA HP

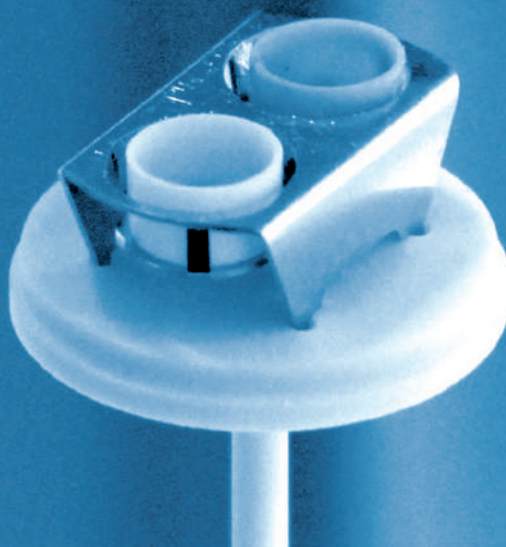

---

Since 1957 LINSEIS Corporation has been delivering outstanding service, know how and leading innovative products in the field of thermal analysis and thermo physical properties.

We are driven by innovation and customer satisfaction.

Customer satisfaction, innovation, flexibility and high quality are what LINSEIS represents. Thanks to these fundamentals our company enjoys an exceptional reputation among the leading scientific and industrial organizations. LINSEIS has been offering highly innovative benchmark products for many years.

The LINSEIS business unit of thermal analysis is involved in the complete range of thermo analytical equipment for R&D as well as quality control. We support applications in sectors such as polymers, chemical industry, inorganic building materials and environmental analytics. In addition, thermo physical properties of solids, liquids and melts can be analyzed.

LINSEIS provides technological leadership. We develop and manufacture thermo analytic and thermo physical testing equipment to the highest standards and precision. Due to our innovative drive and precision, we are a leading manufacturer of thermal Analysis equipment.

The development of thermo analytical testing machines requires significant research and a high degree of precision. LINSEIS Corp. invests in this research to the benefit of our customers.




**Claus Linseis**  
Managing Director



## German engineering

The strive for the best due diligence and accountability is part of our DNA. Our history is affected by German engineering and strict quality control.

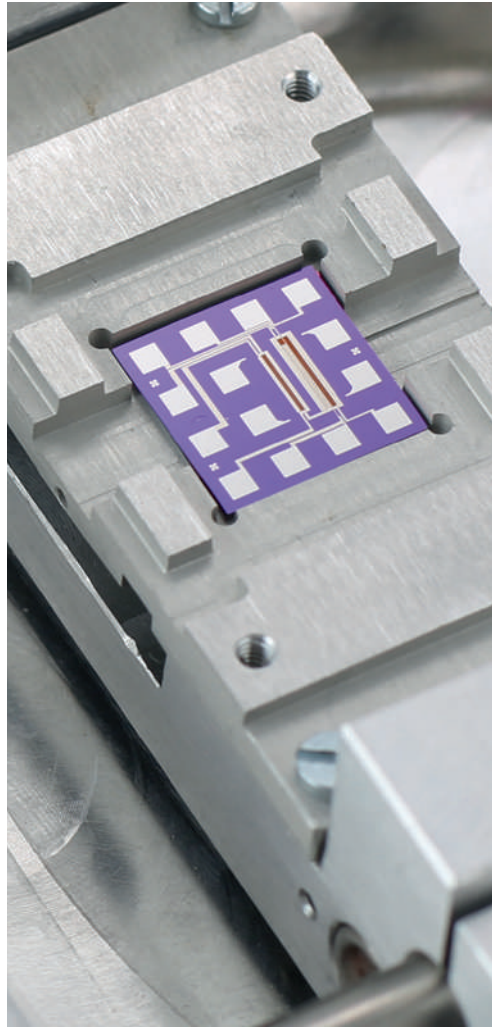

## Innovation


We want to deliver the latest and best technology for our customers. LINSEIS continues to innovate and enhance our existing thermal analyzers. Our goal is constantly develop new technologies to enable continued discovery in Science.

# SIMULTANEOUS THERMAL ANALYSIS

Simultaneous TGA-DTA/DSC measures both, heat flow and weight change of a sample as a function of temperature or time under controlled atmosphere. Simultaneous measurement of these two material properties not only improves productivity but also simplifies interpretation

of the results. The complimentary information obtained allows differentiation between endothermic and exothermic events which have no associated weight change (e.g., melting and crystallization) and those which involve a weight change (e.g., degradation).

## High precision beam balance

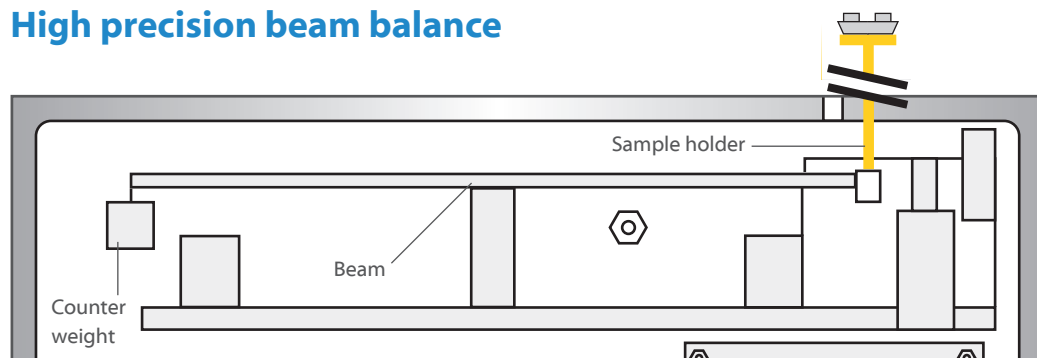

Our different microbalances are specifically designed to accomplish thermal analysis tasks in the best possible way.

Providing ultra light weight design to follow fast weight changes and symmetric construction for ultra low drift long term measurements.

## Advantages of LINSEIS Balance Design



- not affected by local gravity
- not affected by thermal fluctuations
- highest possible PRECISION
- direct measurement of mass
- depending on model, balance can handle mg up to 50g sample mass

## Advantages of combined TG+DSC

- same geometry
- stoichiometry
- same temperature profile
- same atmosphere
- same humidity

# DSC- True Heat Flow measurement

## Quantitative DSC-signal

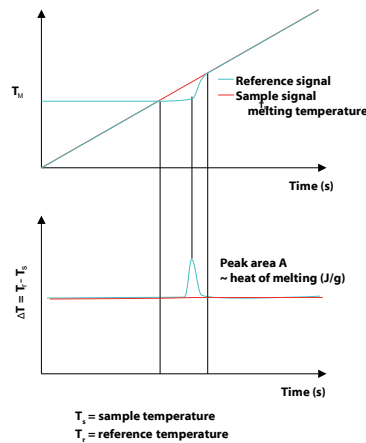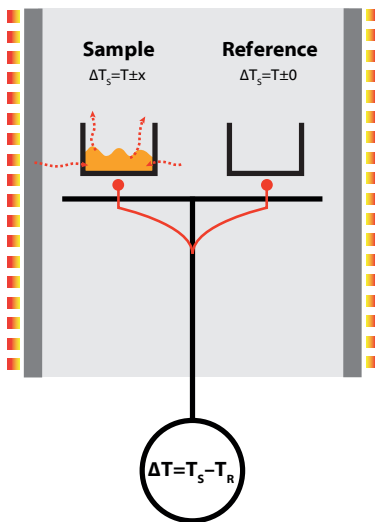

### Differential Scanning Calorimetry (DSC)

"A technique in which the difference in energy input into a substance and a reference material is measured as a function of temperature, while the substance and reference material are subjected to a controlled temperature program."

### Differential Signal

The differential signal is displayed as a baseline. Effects, for example the melting of a metal, can be observed as a peak. The area of the peak gives the amount of enthalpy and the direction of the peak indicates the way of heat flux – endothermic (down) or exothermic (up).

### Temperature vs. Time

During an effect like a reaction, decomposition or phase transition, a temperature difference (heat flux difference) between the sample and the reference crucible can be measured by means of a thermocouple.

## Measurable Properties

- Mass change as % and mg
- Rate controlled mass loss
- Evaluation of mass loss
- Residue mass evaluation
- Compositional analysis


- Enthalpy
- Endo- / Exo- thermic
- Phase transformation
- Melting point
- Glass point
- Crystallinity

- Thermal stability
- Oxidation stability
- Purity
- Solidus / Liquidus relationship
- Product identification


# SENSORS

Our STA can be equipped with an unmatched amount of different user exchangeable TG-DSC, TG-DTA or TG sensors.

Each sensor is available with different thermocouples to provide the highest sensitivity for your desired temperature range.




DSC Heat flux

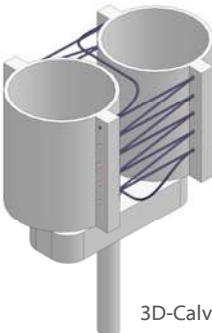


3D-Calvet-DSC sensor

**TG-DSC**


- Al<sub>2</sub>O<sub>3</sub>
- Platinum
- Aluminium
- others



0.12ml




0.12ml



custom volume


Different crucibles available / broad variety

●
●
●
●
●
●
●
●
●



DTA-sensor

- 
- 
-




Cap

0.3ml or custom volume


Crucible

- 
- 
-

**TG-DTA**

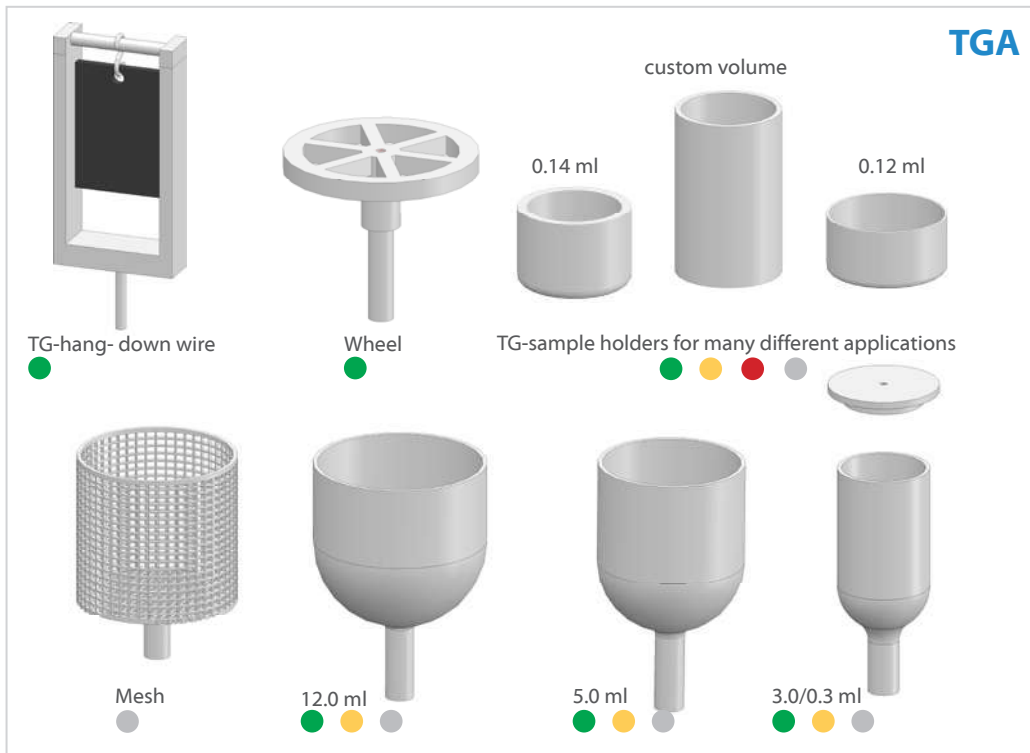


## Best possible sensitivity for your application

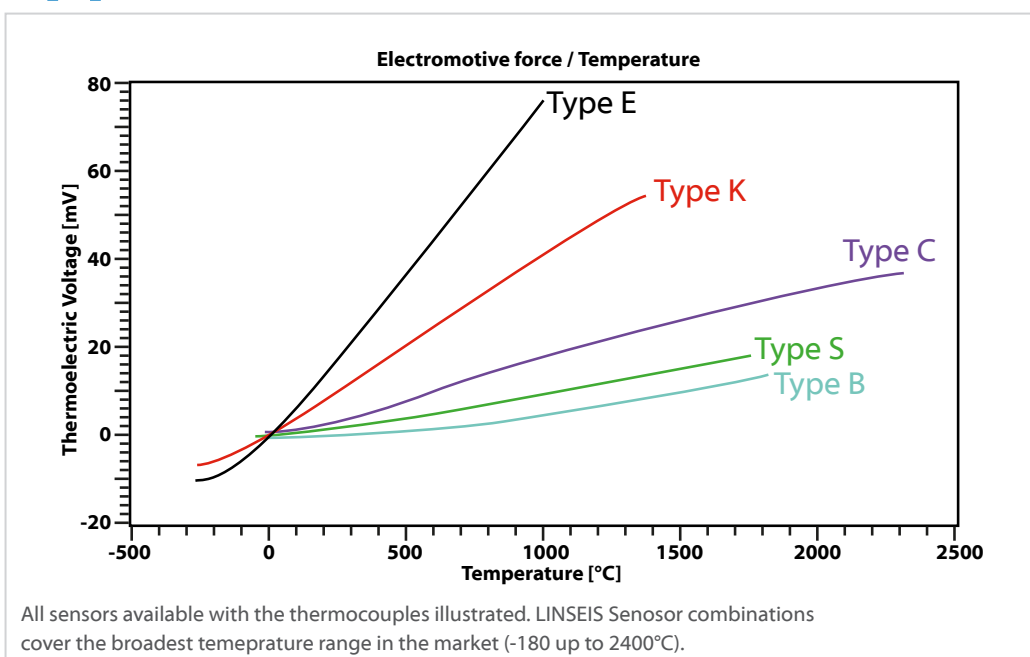

# UNIQUE FEATURES

## Vacuum and controlled atmosphere

The balance design provide for high vacuum, inert, reducing, oxidizing or humidified atmosphere. Furthermore, the instrument can be pressurized up to 5 bar overpressure (option). Certain corrosive conditions can be analyzed with proper precautions. The system is capable of adapting residual gas analysis systems using an optional heated capillary.

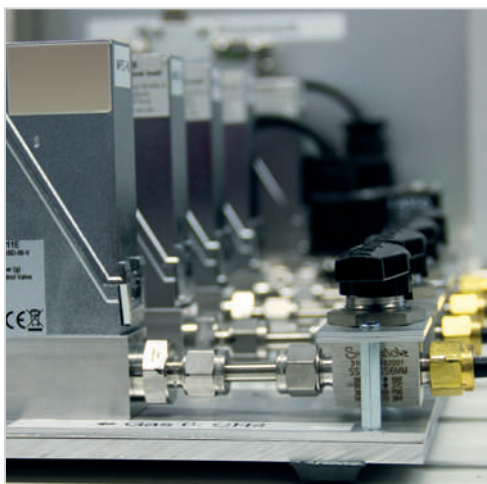

## Evolved gas analysis

Optional gas analysis with MS, FTIR or GCMS is possible. This provides valuable additional information.



## Sample robot

Our STA PT 1000 and 1600 can be equipped with a proven sample robot for unattended sample measurements.

## Wide temperature range -150 to 2400°C

The LINSEIS STA instruments can be equipped with up to two furnaces at the same time. A broad variety of different furnaces is available to enable measurements in the widest temperature range on the market. Unmatched selection of furnaces for widest possible temperature range.







## Starter kit

The starter kit includes a variety of tools such as scissors, cutting tools, anti electrostatic tweezers, magnifier, crucible holder, pipette, rasps, spatula etc.


## Oxygen Getter Material OGM

The LINSEIS oxygen getter system (OGM) can be placed in any LINSEIS system as a modification

of the sample gas capillary. It is used to getter smallest traces of residual oxygen in the sample chamber by offering a stronger oxygen affinity than sample materials, combined with a high effective surface to ensure the oxygen molecules react with the getter before they have a chance to get in touch with the sample. Especially for oxidation sensitive samples, where hydrogen gas mixtures can't be used or very small enthalpy signals are expected, the OGM is a very effective and easy to use solution. With its modular character, it can be used for special experiments and can be easily removed for measurements under air or where the oxygen content is less important.


## Furnace Programm

Temperature	Type	Element	Atmosphere	TC-Type
-150 -- -500°C	L81/264	Kanthal	inert, oxid., red., vac.	K
-150 – 1000°C	L81/264ER	Kanthal	inert, oxid., red., vac.	K
RT – 1000°C	L81/220	Kanthal	inert, oxid., red., vac.	K
RT – 1200°C	L81/IR	IR Heater	inert, oxid., red., vac.	S
RT – 1500°C	L81/230Pt	Precious Metal	inert, oxid., vac.	S
RT – 1600°C	L81/240	SiC	inert, oxid., vac.	S
RT – 1650°C	L81/240Rh	Precious Metal	inert, oxid., vac.	B
RT – 1750°C	L81/250	MoSi <sub>2</sub>	inert, oxid., vac.	B
RT – 2000°C	L81/260	Graphite	inert., red.	C
RT – 2400°C	L81/260	Graphite	inert., red.	C
<b>Special Furnaces</b>				
RT – 1600/1750°C	L81/240/250 WV	SiC/MoSi <sub>2</sub>	water vapor furnace	
RT – 1100/1600°C	L81/IR/HF	IR/HF	high speed furnaces up to 100°C/s	

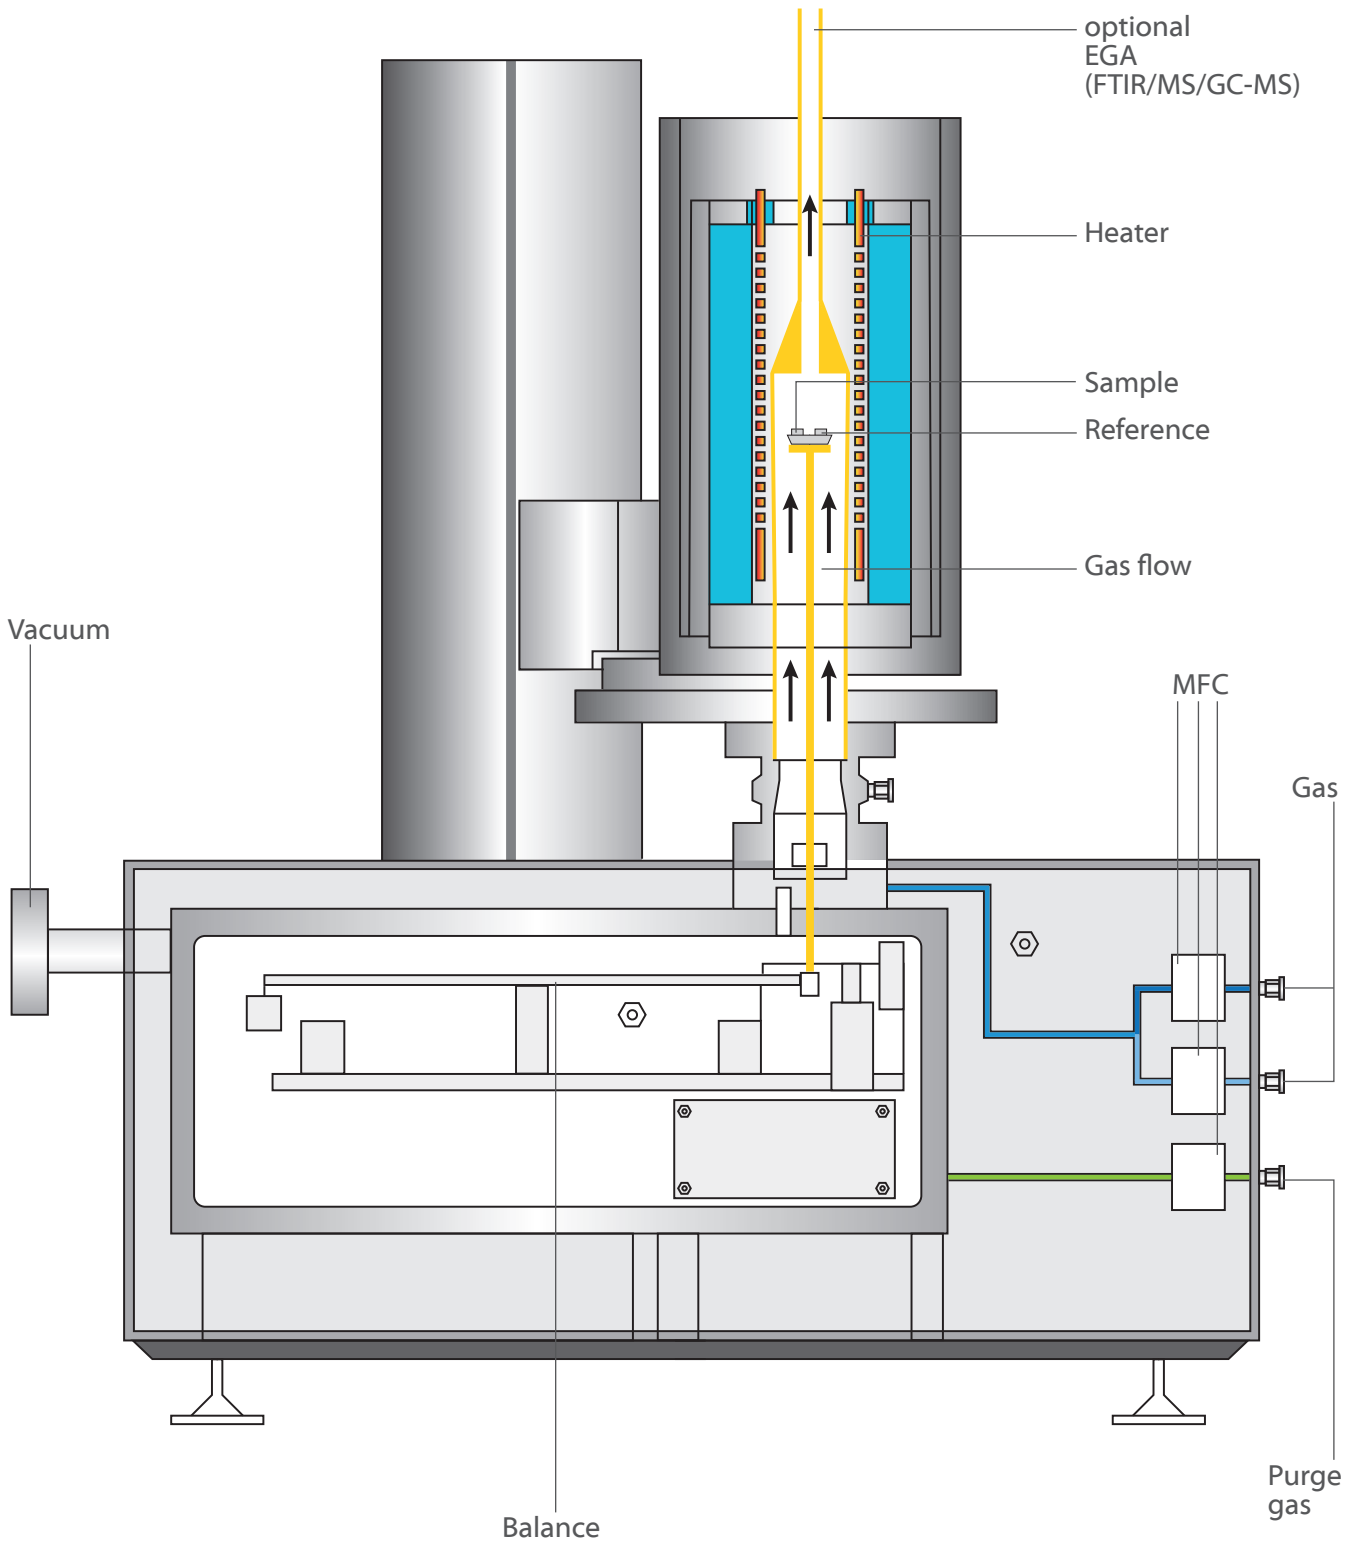

# Benefits of the vertical top loading design

The vertical “sample on top” design of the LINSEIS thermobalance provides highest possible accuracy due to a stable position of the sample and easy sample handling.

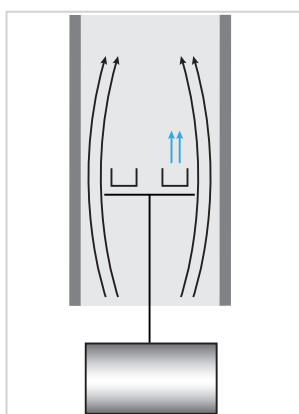

## Vertical system (sample on top)

### LINSEIS configuration

Advantages:

- Easy sample handling
- Easy exchange of sample holder
- Stable position of the sample in the furnace (critical for good DTA/DSC and Cp results)

Disadvantage:

- Complicated construction



## Horizontal system

Advantages:

- Small buoyancy effects

Disadvantages:

- Sensor exchange very difficult
- Sample handling difficult
- Very high purge gas rate required
- Problems due to sensor expansion during heating/cooling

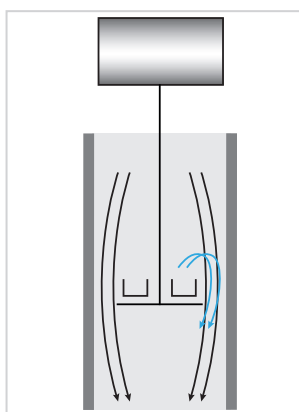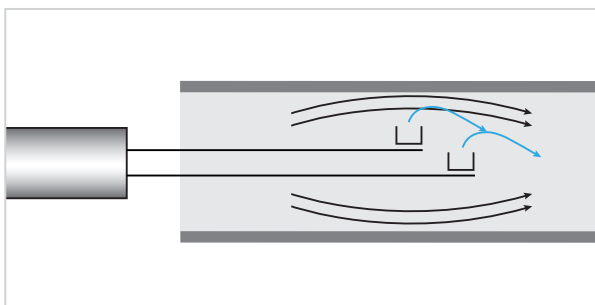

## Vertical system (sample on bottom)

Advantage:

- Stable position within furnace

Disadvantages:

- Difficult sensor exchange
- “Dangerous” gas flow within balance housing (sample gets blown out)
- Sensor position depends on sample weight

---

# STA PT 1000

## Compact fully integrated TG-DSC/DTA for organic materials

The STA PT1000 is dedicated to analysis of organic materials in a relatively low temperature range up to 1000°C.

The LINSEIS HiRes option for TGA allows analyzing mass change effects with highest possible accuracy by effective trigger heating rate changes. The software can detect a mass change that could be due to oxidation or decomposition. As a result the unit can automatically adjust the heating rate or stop heating. After the mass change is over, the system continues heating according to the set profile. This allows a better separation of effects that are taking place

shortly after each other or almost similar. The LINSEIS STA PT 1000 has an integrated furnace control cycle that enables the system to stop heating and perform heating rates with a minimum of overshooting so that a broad range of applications can be covered with the HiRes software option.

### Design

build in furnace and gas control  
furnace with low thermal mass for unmatched heating and cooling speed

### Sample robot

optional 42 or 84 position sample robot is available



---

# STA PT 1600

## STA PT 1600/1

The highest resolution 0.025 µg balance for small sample quantities allows the detection of very small effects with highest accuracy.

## STA PT 1600/2

The standard model covers a broad application range with excellent resolution 0.1 µg and accuracy.

## STA PT 1600/3


The high mass variant allows measuring samples with big volumes or weight 35/50g to determine even small effects within a big amount of inhomogeneous material.

**TG - DSC/DTA + Pressure**



---

# STA HIGH PRESSURE

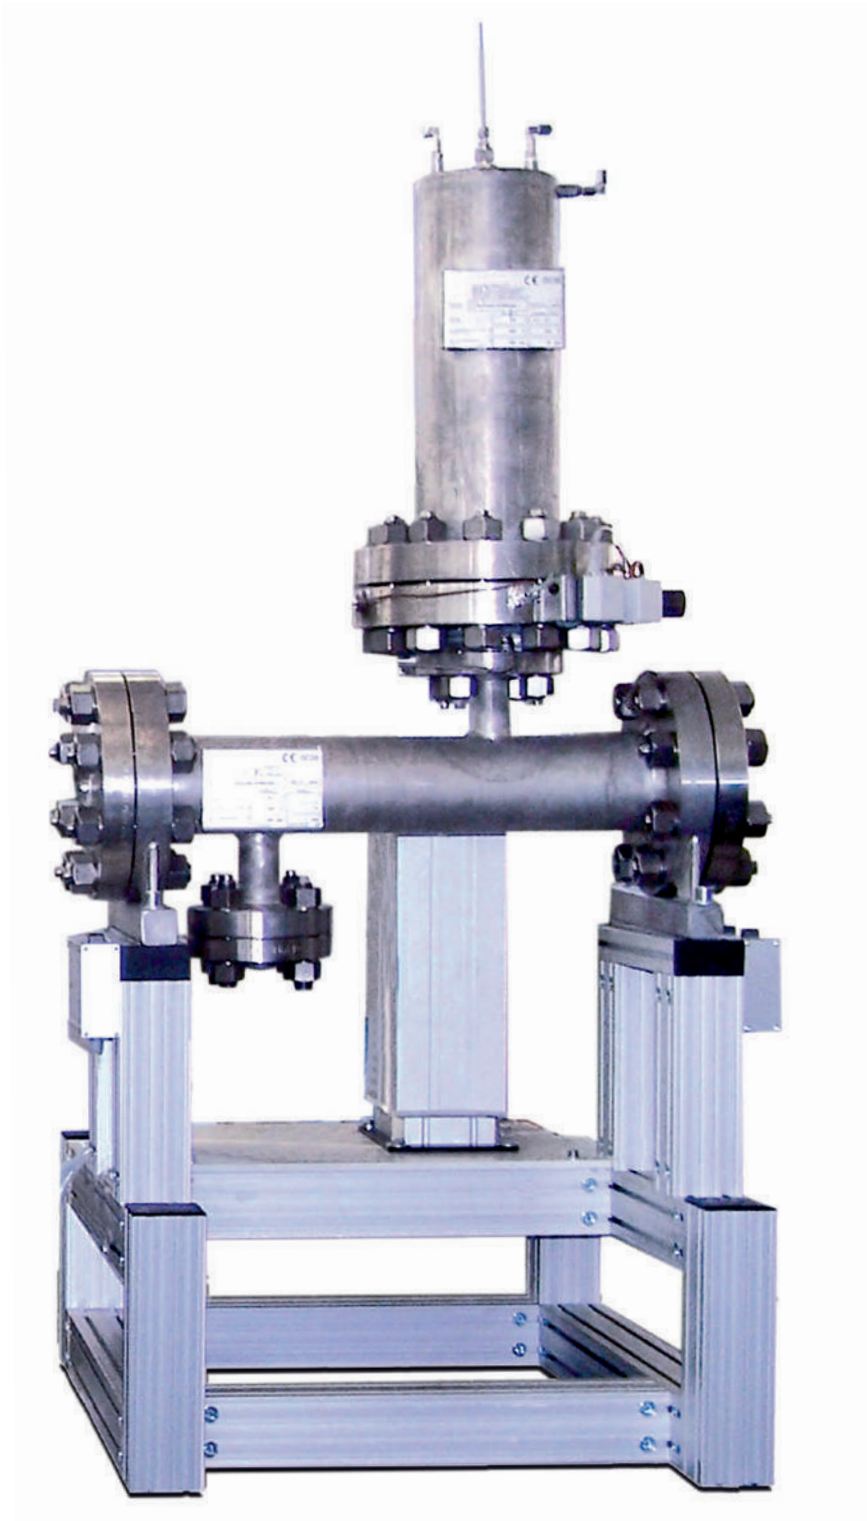

# High pressure & high temperature

Taylor made STA product for challenging custom applications


## Measurement System

The LINSEIS STA HP thermobalances are the only system available on the market to provide TG and DTA/DSC data under pressurized conditions from -150 up to 1800°C. The instrument offers a broad range of TG, TG-DTA and TG-DSC measuring systems which are easily exchangeable.

## Unique Features

### Vacuum, Vapor and Controlled Atmosphere

The balance design provides for high vacuum ( $10^{-4}$ mbar), inert, reducing or hulfimified atmosphere under static or flowing gas atmosphere. Corrosive conditions can be analyzed with proper precautions. A unique gas control for high pressure applications is available to ensure smooth gas flow switching under pressure conditions without affecting the TG signal. Furthermore, a sophisticated vapor generator can be supplied with the equipment.

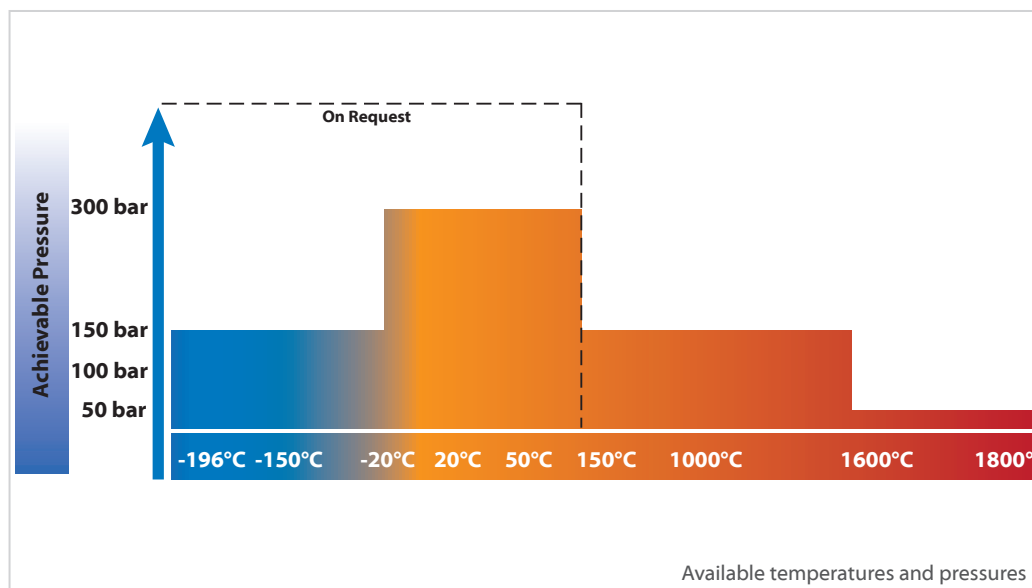

TG - DSC/DTA + Pressure

"Opens the door to new research possibilities"

# SOFTWARE

All LINSEIS thermo analytical instruments are software controlled. The individual software modules run exclusively under Microsoft® Windows® operating systems. The complete software consists of 3 modules: temperature control, data acquisition and data evaluation. The Windows® software incorporates all essential features for measurement preparation, execution and evaluation of a thermoanalytical measurement. Thanks to our specialists and application experts, LINSEIS was able to develop comprehensive easy to understand user friendly application driven software.

## Features-Software:

- Program capable of text editing
- Data security in case of power failure
- Thermocouple break protection
- Repetition measurements with minimum parameter input
- Evaluation of current measurement
- Curve comparison up to 32 curves
- Storage and export of evaluations
- Export and import of data ASCII
- Data export to MS Excel
- Multi-methods analysis (DSC TG, TMA, DIL, etc.)
- Zoom function
- 1 and 2 derivation
- Programmable gas control
- Curve arithmetics
- Statistical evaluation package
- Free scaling


- Optional Kinetic and Lifetime Prediction
- Software packages

## TG – Features:

- Mass change as % and mg
- Rate Controlled Mass Loss (RCML)
- Evaluation of mass loss
- Residue mass evaluation

## HDSC – Features:

- Glass transition temperature
- Complex peak evaluation
- Multipoint calibration for sample temperature
- Multipoint calibration for change of enthalpy
- Cp calibration for heat flow
- Signal-steered measuring procedures

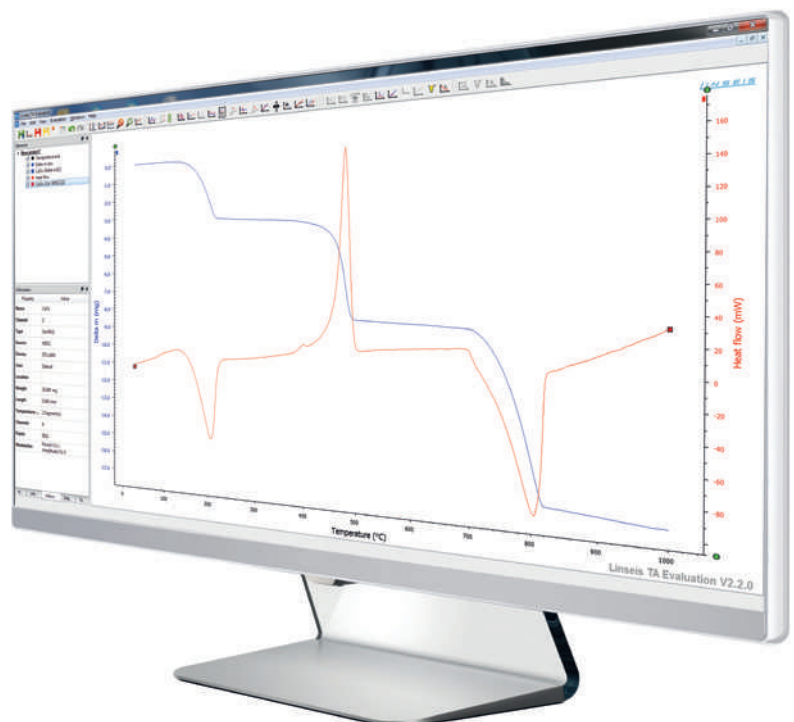




## Thermal Library

The LINSEIS Thermal Library software package comes as an option for the well-known, user friendly LINSEIS Platinum evaluation software that is integrated in almost all our instruments.

The Thermal Library allows you the comparison of the complete curves with a data base providing thousands of references and standard materials within only 1-2 seconds.

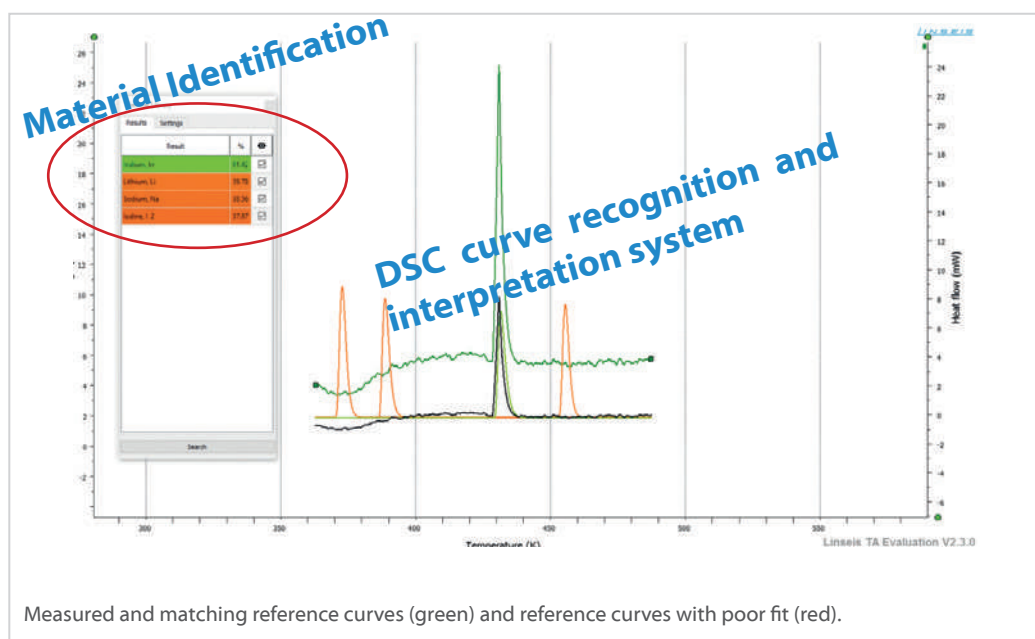

## Multi-Instrument

All LINSEIS instruments DSC, DIL, STA, HFM, LFA, etc. can be controlled from one software template.

## Report Generator

Convenient template selection to generate customized measurement reports.

## Data Base

State of the art data base design enables easy data handling.

## Multi-Lingual

Our software is available in many different user exchangeable languages, such as: English, Spanish, French, German, Chinese, Korean, Japanese, etc.

## Multi-User

The administrator can generate different user levels providing different rights to operate the instrument. An optional Log file is available, too.

## Kinetic software

Kinetic analysis of DSC, DTA, TGA, EGA (TG-MS, TG-FTIR) data for the study of the thermal behavior of raw materials and products.

---

# OTS OXYGEN GETTER



For very sensitive samples and experiments where surface oxidation is critical, LINSEIS is providing an oxygen getter system OST for STA, TGA, DSC and Dilatometers, that can be easily added as an additional option to the mentioned methods. The OST consists of a special Zirconium alloy and reduces the residual oxygen content in inert atmospheres down to very low ppm levels. It is installed by just plugging it on top of the standard gas capillary. During the first use it will be welded onto the capillary and can then be used for many cycles.

## Features:

We recommend using the LINSEIS OST only with pure gases with purity grade 4.7 or higher. For the optimal getter effect, the used gas should be Argon or Helium.

- high reactive surface for maximum activity
- usage from RT to 1600°C
- easy to use, modular design
- designed for ultra-pure inert atmospheres
- not toxic and not corrosive


# TECHNICAL SPECIFICATIONS

	STA PT 1000	STA PT 1600			STA HP/2	
<b>Temperature range</b>	RT up to 1000°C	-150 up to 2400°C			RT up to 1100/ 1400°C/1600°C/1800°C	
<b>Vacuum</b>	optional 10 <sup>-2</sup> mbar	10 <sup>-5</sup> mbar (depends on vacuum pump)			up to 10 <sup>-4</sup> mbar	
<b>Pressure</b>		up to 5 bar (optional)			up to 150 bar custom solution on request	
<b>Heating rate</b>	0.01 up to 100K/min	0.01 up to 100K/min (depends on furnace) (from 0.001°C/min on request)			0.01 up to 100K/min	
<b>Temperature precision</b>	0.001°C	0.001°C			0.05°C	
<b>Sample robot</b>	optional 42 / 84	optional 42			-	
<b>TG</b>		<b>1</b>	<b>2</b>	<b>3</b>		
<b>Resolution</b>	0.1 µg	0.025 µg	0.1 µg	0.1 µg	0.1 µg	0.1 µg
<b>Sample weight</b>	5 g	5 g	25 g	35 / 50 g	15 / 25 g	35 / 50 g
<b>Measuring range</b>	25 / 2500 mg	25 / 2500 mg	25 / 2500 mg	35000 mg	25 / 2500 mg	35000 mg
<b>DSC</b>						
<b>DSC-sensors</b>	E / K / S	E / K / S / B / C (C = DTA only)			E / K / S / B / C	
<b>DSC resolution</b>	0.3 / 0.4 / 1µW	0.3 / 0.4 / 1 / 1.2 µW			0.3 / 0.4 / 1 / 1.2 µW	
<b>Calorimetric sensitivity</b>	approx. 4 / 6 / 17.6 µW	approx. 4 / 6 / 17.6 / 22.5 µW			approx. 4 / 6 / 17.6 / 22.5 µW	
<b>DTA</b>						
<b>DTA-resolution</b>	0.05 µV	0.05 µV			0.05 µV	
<b>Sensitivity</b>	1.5 µV/mW	1.5 µV/mW			1.5 µV/mW	
<b>DTA-measuring ranges</b>	250 / 2500 µV	250 / 2500 µV			250 / 2500 µV	

# APPLICATIONS


# STA PT 1000

## Decomposition of rubber

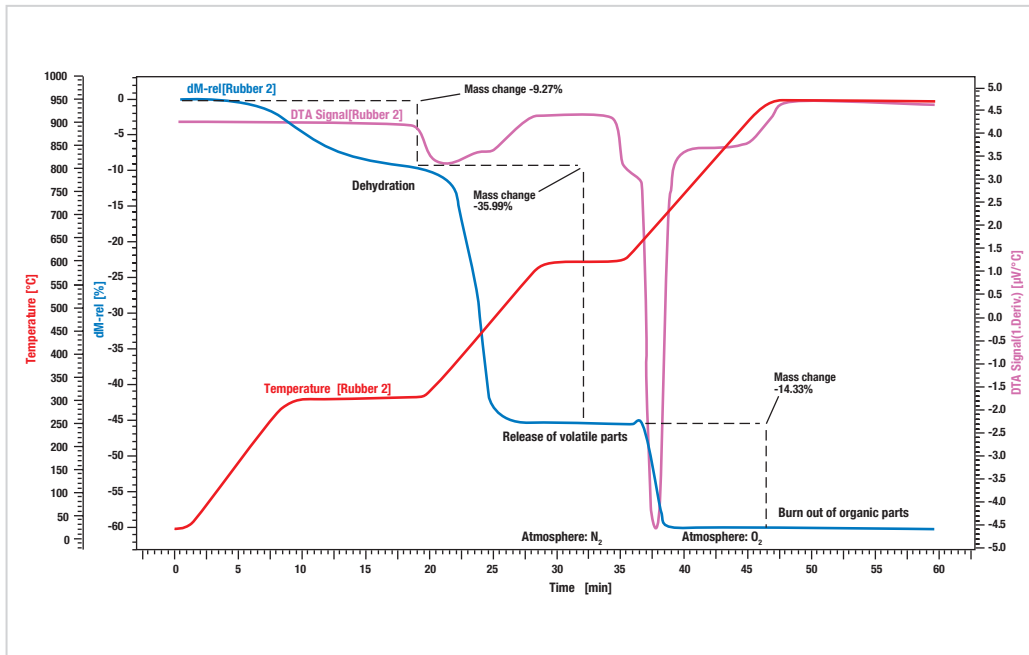

In the first step of weight loss, the dehydration of the sample takes place. The amount of water was 9.27%. In the second reaction step, the volatile components are released by pyrolysis under N<sub>2</sub> atmosphere. The amount of these components is 35.99%. For the third reaction step, the atmosphere is changed to O<sub>2</sub> – all organic components are burned out. The loss in weight is 14.33%. The remaining 40.41% are inorganic components like ashes, slake or fillers.


## Aspirin

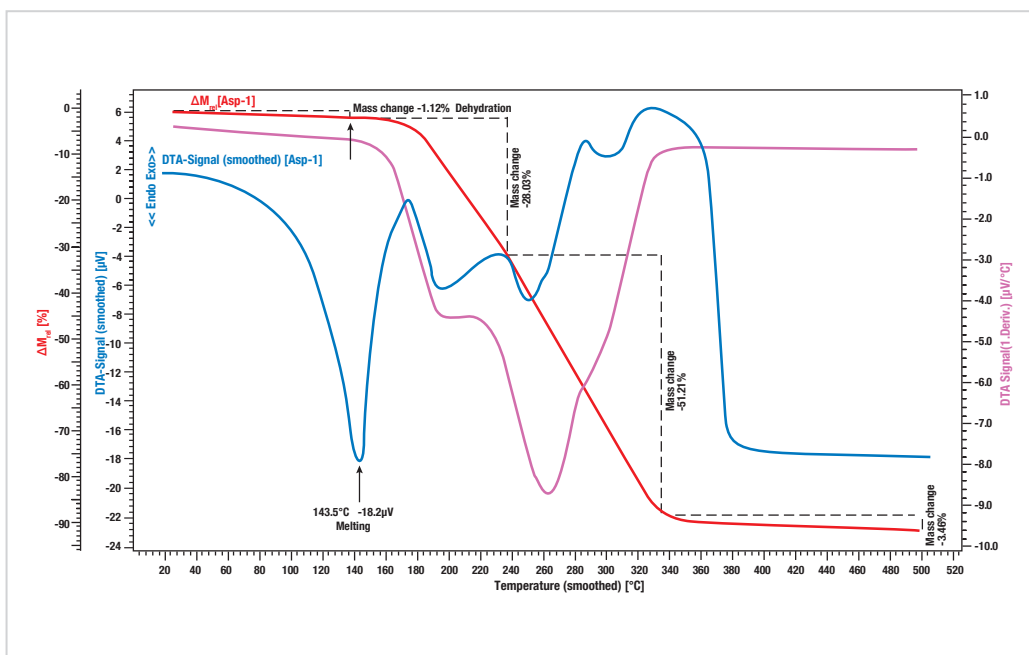

At the beginning of the heating process some adsorbed water is released, resulting in a weight loss of around 1%. At 140°C the melting point of the Aspirin is reached, resulting in an endothermic reaction, measured on the DTA trace. At 160°C the decomposition of the melted drug takes place in several stages. The decomposition products are volatile thereby giving a total weight loss of almost 100%.


# STA HP

## Hydrogen Adsorption on Titanium at 700°C

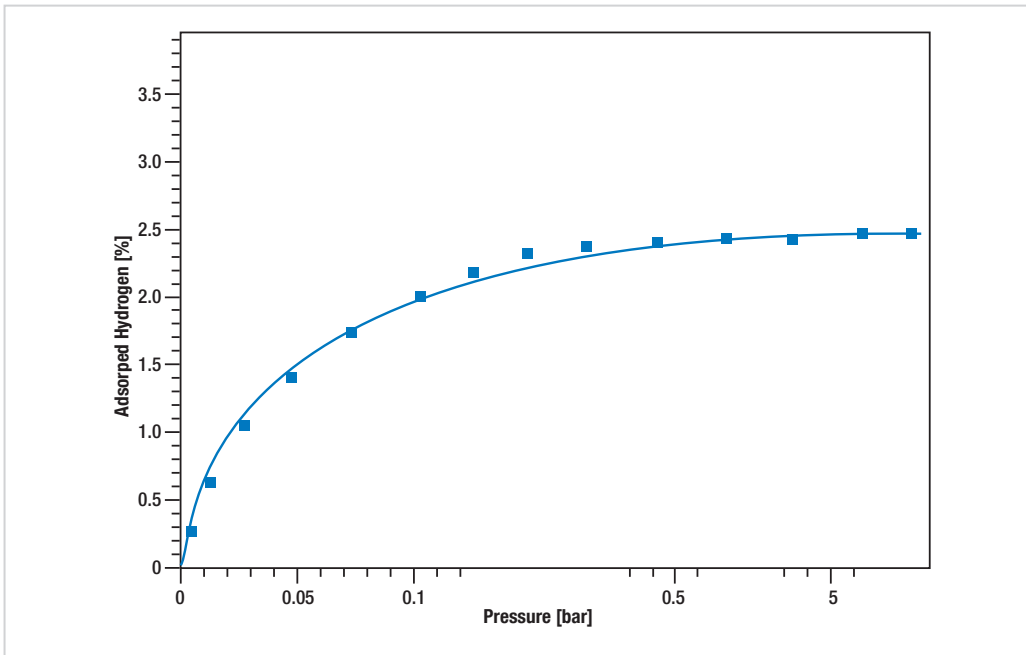

Activated, porous titanium surface was heated to 700°C under vacuum. At target temperature, hydrogen was added and the pressure was increased in an isothermal stage. The weight increase of the sample gives the amount of hydrogen that is adsorbed on the titanium surface over pressure, leading to saturation (2.5% weight) at 5 bar.


## Coal gasification

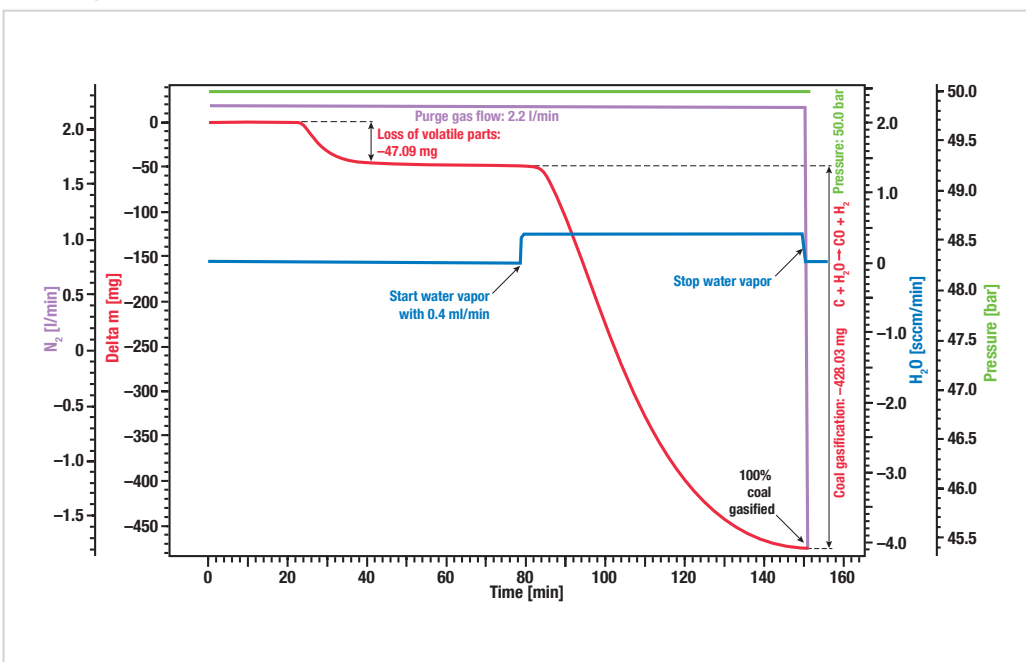

Coal was heated under nitrogen atmosphere at 50bar pressure. The mass signal shows the loss of volatile components between 20 and 40min. After water vapor was added, the coal was gasified and nearly completely consumed after 150min, leading to H<sub>2</sub>, CO, CH<sub>3</sub>OH and other useful reactive gases.


# STA PT 1600

## Decomposition of $\text{CaC}_2\text{O}_4 \cdot \text{H}_2\text{O}$

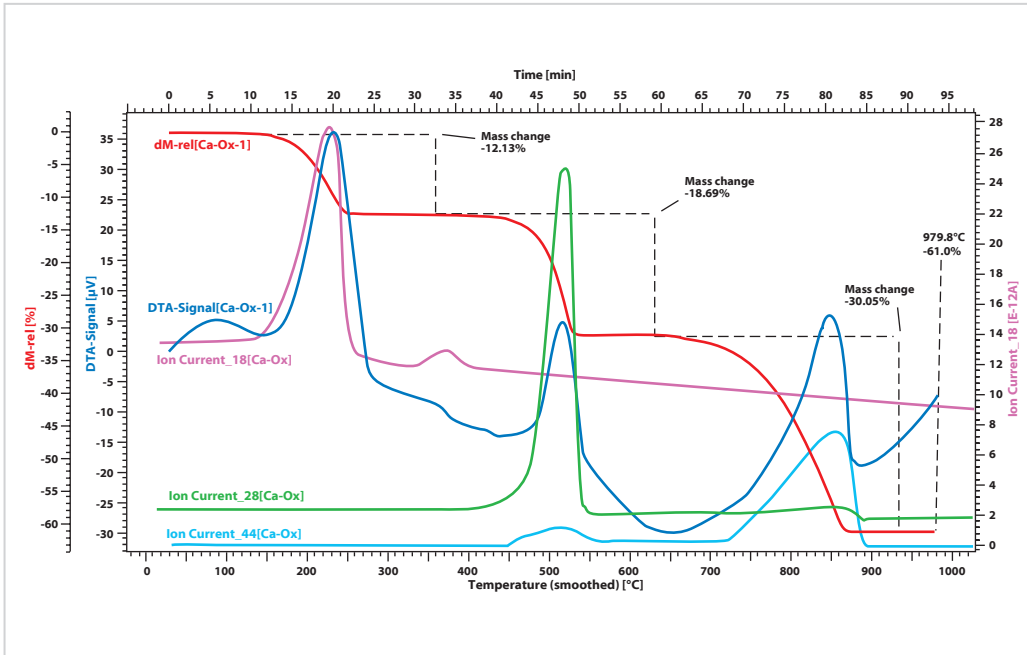


The evolved gases from the decomposition of calcium oxalate has been fed into the mass spectrometer with a heated capillary. The ion currents for mass numbers 18 (water), 28 (carbon monoxide) and 44 (carbon dioxide) have been imported into the graph.

## Cement

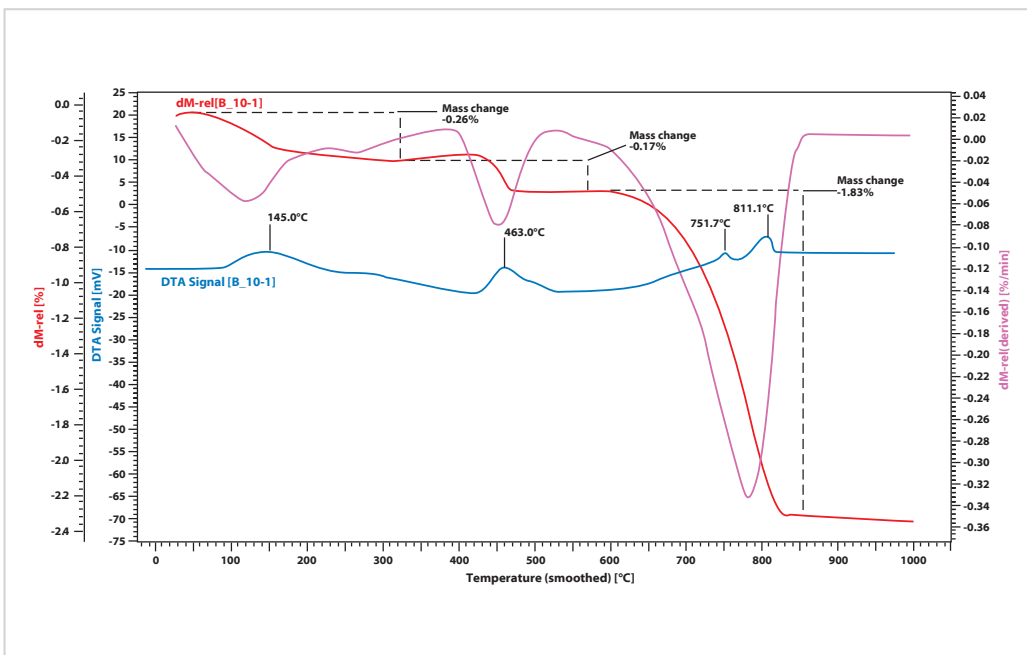


The main parts of cement are tri calcium silicate, di calcium silicate and tri calcium aluminates. Hydrates slowly form after mixing cement with water. The absorbed water evaporates first. Hydrates of the calcium silicate decompose at 570°C. The hydroxides of calcium, magnesium and aluminum follow. Subsequently,  $\text{CO}_2$  splits off from calcium carbonate.

## Long term baseline stability

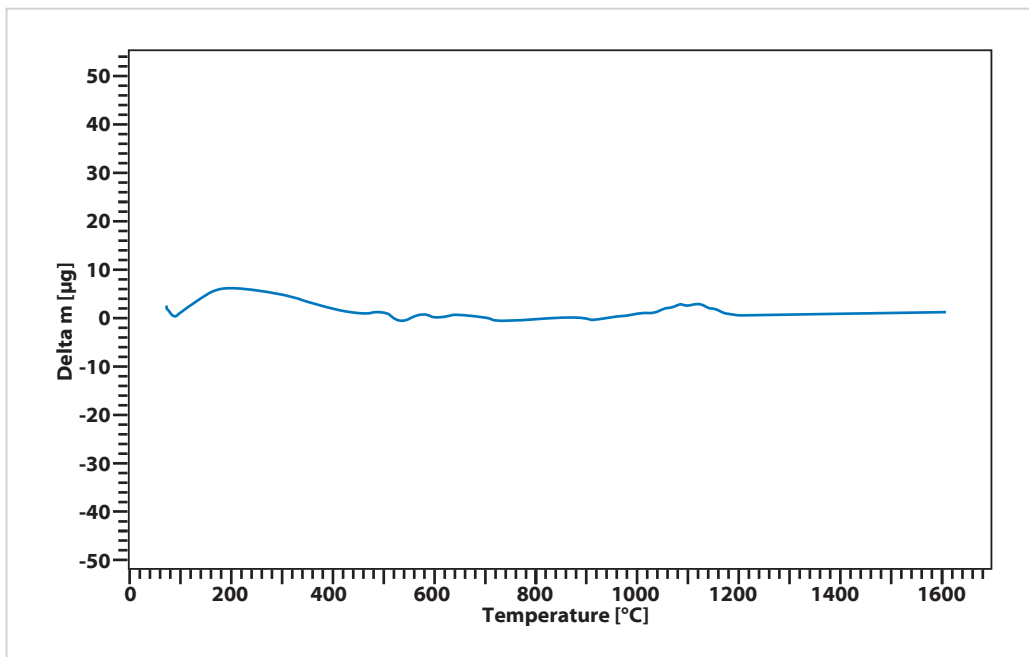

The average baseline stability during linear heating up to 1600°C is within a range of 5µg. This allows highest accuracy and repeatability during the most demanding applications on STA.

## Modulated $c_p$ determination

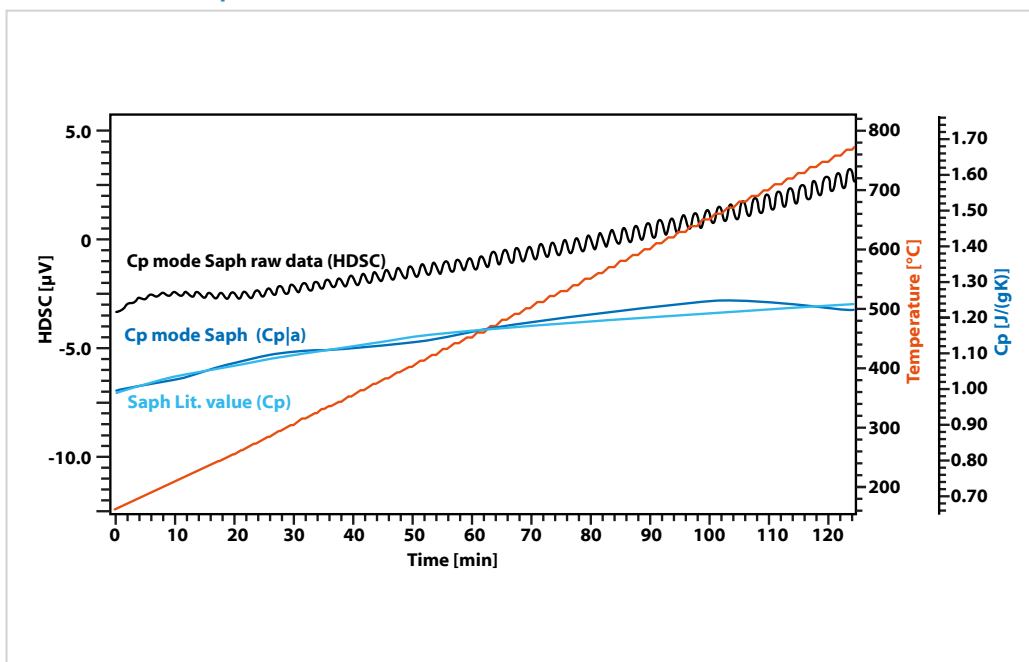

For highest possible accuracy of  $C_p$ , the LINSEIS STA and DSC allow the usage of modulated temperature profiles. This technique causes a continuous change in heat flow of the sample and the system can monitor the heat uptake much better than with a linear heating profile. The deviation from the literature value is much smaller than with non-modulated DSC profiles. The modulated heat flow signal (black) leads to a significant better  $C_p$  data (dark blue) that is only slightly different from literature (bright blue). The orange curve shows the modulated temperature signal.

**LINSEIS GmbH Germany**

Vielitzerstr. 43

95100 Selb

Tel.: (+49) 9287 880 0

E-mail: info@linseis.de

**LINSEIS Inc. USA**

109 North Gold Drive

Robbinsville, NJ 08691

Tel.: (+1) 609 223 2070

E-mail: info@linseis.de

**LINSEIS China**

Kaige Scientific Park 2653 Hunan Road

201315 Shanghai

Tel.: (+86) 21 5055 0642

Tel.: (+86) 10 6223 7812

E-mail: info@linseis.de

**LINSEIS France**

1 Route de Trévoux

69250 Neuville/Saone

Tel.: (+33) 6.24.72.33.31

E-mail: contact@ribori-instrumentation.com

**LINSEIS Poland**

ul. Dabrowskiego 1

05-800 Pruszków

Tel.: (+48) 692 773 795

E-mail: info@linseis.de

**[www.linseis.com](http://www.linseis.com)****Products:** DIL, TG, STA, DSC, HDSC, DTA, TMA, MS/FTIR, In-Situ EGA, Laser Flash, Seebeck Effect, Thin Film Analyzer, Hall-Effect**Services:** Service Lab, Calibration Service

01/20

**LINSEIS**